


Startfrequenz: 0.000000 MHz; Endfrequenz: 159.997994 MHz; Schrittweite: 32.006 kHz

Messpunkte: 5000; Zwischenzeit: 0 uSek

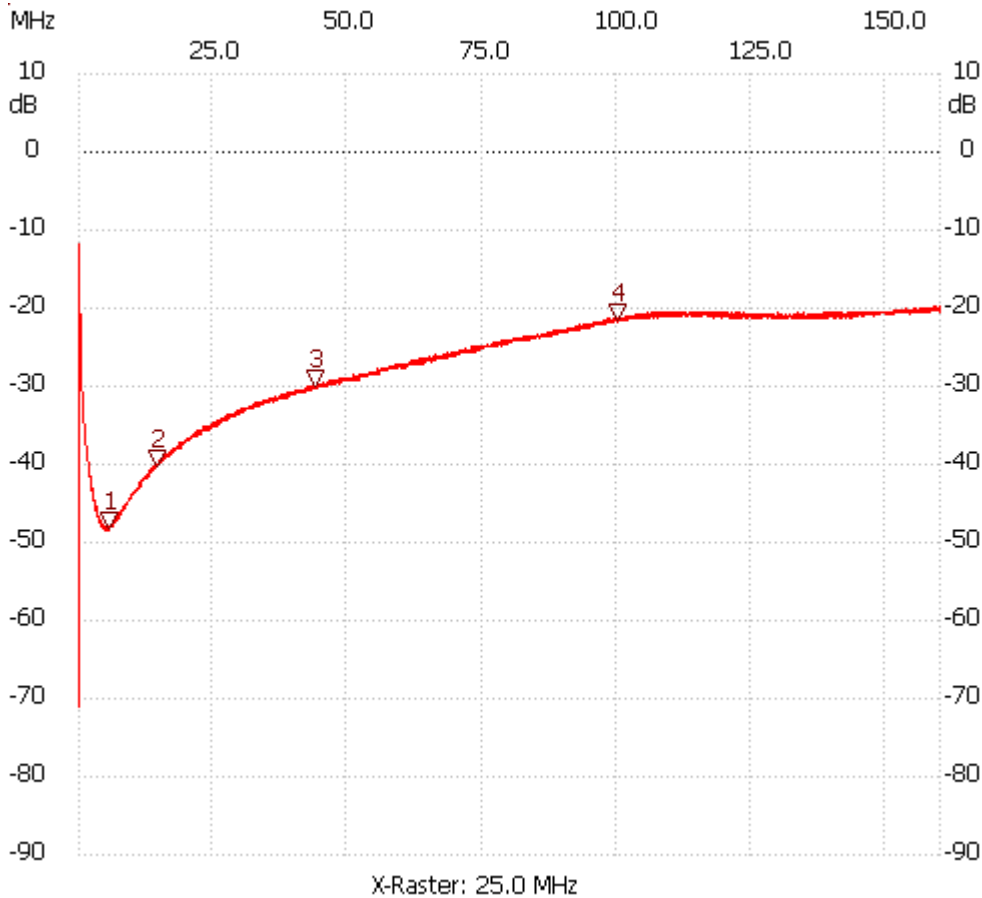

Circulator/Isolator AD8000

min:-71.15dB 0.000000MHz

Kursor 1:

5.473026 MHz

Kanal1: -48.25dB

Kursor 2:

14.498718 MHz

Kanal1: -40.30dB

Kursor 3:

43.784208 MHz

Kanal1: -30.09dB

Kursor 4:

99.954738 MHz

Kanal1: -21.57dB

Kanal 1

max:-10.22dB 0.000000MHz