


HAMEG Instruments

Measure time: 10:13:46
Measure date: 06.09.2007

CH1: 1,000V/DIV DC CH2: 5,000V/DIV DC TB A: 5 μ s TR: CH2+DC PT:-75

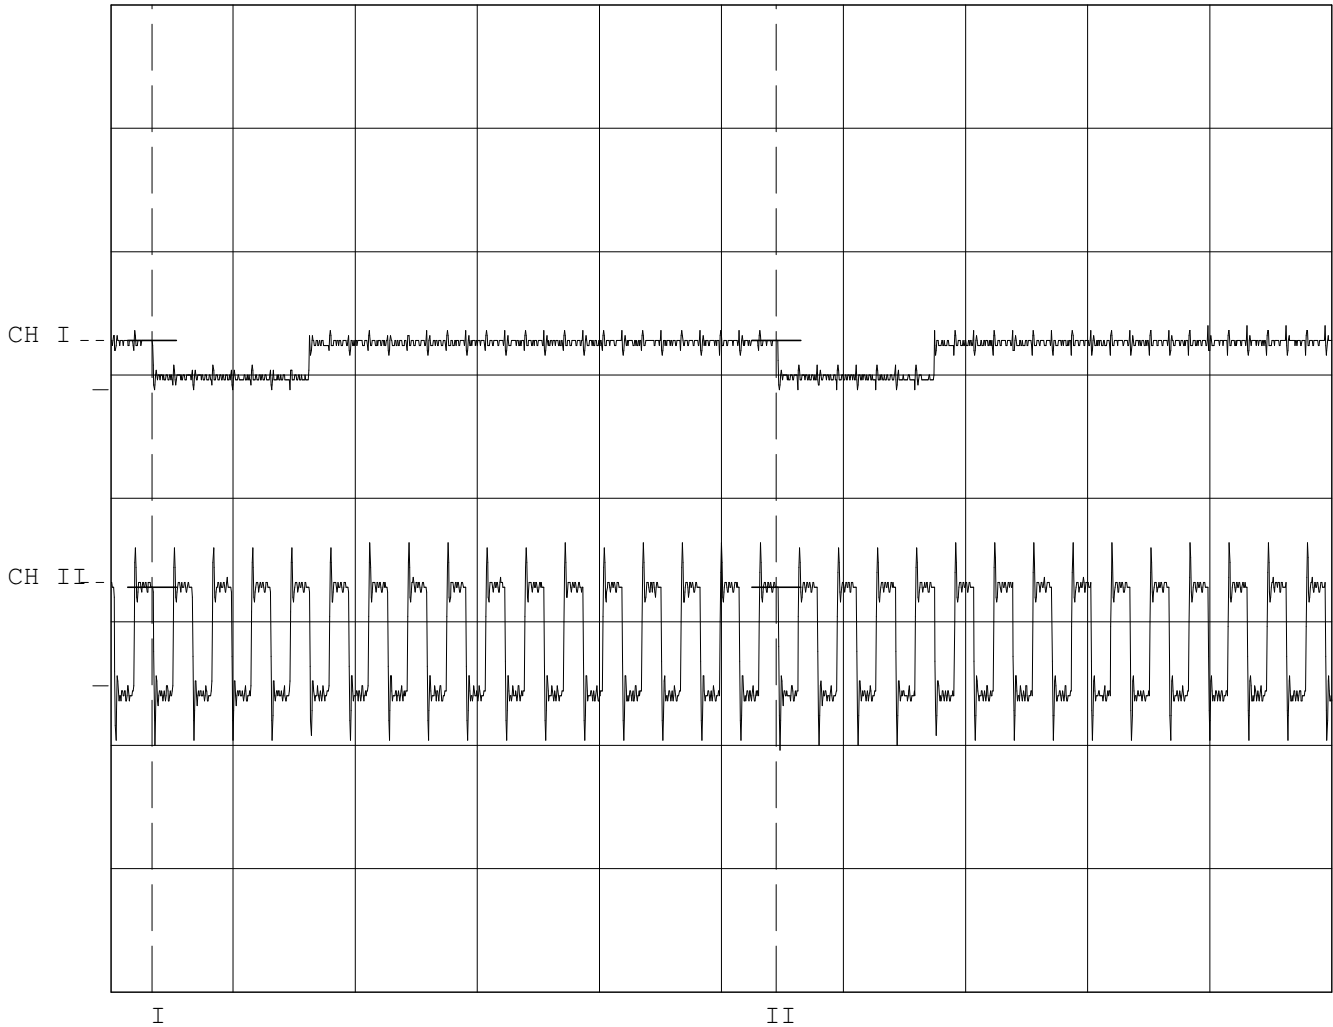

CH I : Cursor I: ,400V Cursor II: ,400V Diff. I-II: ,0000V
CH II: Cursor I: 4,000V Cursor II: 4,000V Diff. I-II: ,0000V

dt: 25,575 μ s 1/dt: 39,101 kHz

Notes: